


# MULTI-UNIT DASSYSTEM

Work different, work better



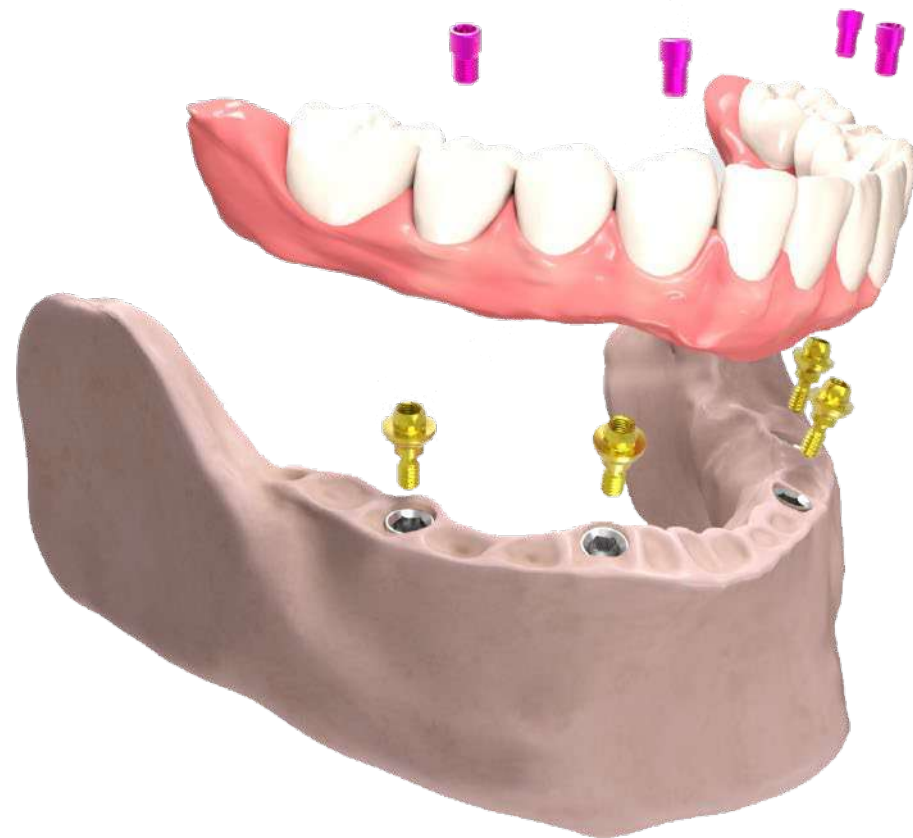

## LIST OF COMPATIBILITIES AVAILABLE

AB	DIO IMPLANTS	NOBEL BIO CARE
ACE	EASY IMPLANT	NORIS MEDICAL
ADIN	EUROTEKNIKA	OSTEOPLUS
ALPHABIO	GLOBAL D (TEKKA)	OSSTEM IMPLANT
ANCLADEN	HAHN IMPLANT (GLIDEWELL)	PALTOP
ANKYLOS	HI-TEC	PROCLINIC
ARDS	HIOSEN	SEWON MEDIX
ASTRA	IBS	SGS
AVINENT	IDO IMPLANTS	SIGNO VINCES
BEGO	IHDE DENTAL (IMBIODENT)	SIN IMPLANTS
BIOCONCEPT	IMPLANT DIRECT	SOUTHERN IMPLANTS
BIOGENESIS	IMPLANT GENESIS	STRAUMANN
BIOHORIZONS	INTRA-LOCK	TITANIUM - FIX
BIOMET 3i	JDENTALCARE	TRE-OSS
BIONER	LEADER	TRI DENTAL IMPLANTS
BIOTEC	MEDENTIS	UFIT
BTK	MEGAGEN	VULKAN IMPLANTS
B&W	MIS	XIVE
CAMLOG	MOZO-GRAU	YES IMPLANT
CONEXÃO SISTEMA DE PRÓTESE	MPI	ZIMMER
CORTEX	NEODENT	
DENTIUM	NEOBIOTECH	

AB

✱ I2	
Implant: Ø 3,5/3,75/4,2/4,5/ 5/6 Platform: Standard (Code 0040)	p.26
✱ I22	
Implant: Ø 3,75/4,22 Platform: Standard (Code 0040)	p. 26
✱ I5	
Implant: Ø 3,5/3,75/4,2/4,5/5/6/7/8 Platform: Standard (Code 0040)	p. 26
✱ I55	
Implant: Ø 3,75/4,2/4,5/5/6/7/8 Platform: Standard (Code 0040)	p. 26
✱ I10	
Implant: Ø 4,2/5 Platform: Standard (Code 0040)	p. 26
✱ I15	
Implant: Ø 6/7/8 Platform: Standard (Code 0040)	p. 26

ACE

✱ Infinity Internal Hex	
Implant: Ø 3,7/4,1 Platform: 3,5 (Code 0040)	p. 26

ADIN

✱ Swell	
Implant: Ø 3,3 Platform: 3,45 (Code 0040)	p. 26
Implant: Ø 3,75/4,2 Platform: 3,6 (Code 0040)	p. 26
Implant: Ø 5 Platform: 4 (Code 0040)	p. 26
Implant: Ø 6 Platform: 4,6 (Code 0040)	p. 26

✱ Touareg-S / Touareg-OS

Implant: Ø 3,5 Platform: 3,45 (Code 0040)	p. 26
Implant: Ø 3,75/4,2 Platform: 3,6 (Code 0040)	p. 26
Implant: Ø 5 Platform: 4 (Code 0040)	p. 26
Implant: Ø 6 Platform: 5 (Code 0040)	p. 26
✱ Touareg CloseFit	
Implant: Ø 3,5 Platform: RP (Code 0021)	p. 24

ALPHABIO

✱ Internal Hex Connection (IH) SPI	
Implant: Ø 3,3/3,75/4,2/5/6 Platform: Universal (Code 0040)	p. 26
✱ Internal Hex Connection (IH) ICE	
Implant: Ø 3,7/3,75/4,2/4,65/5,3 Platform: Universal (Code 0040)	p. 26

✱ Internal Hex Connection (IH) DFI	
Implant: Ø 3,3/3,75/4,2/4,5 Platform: Universal (Code 0040)	p. 26

✱ Internal Hex Connection (IH) ATID	
Implant: Ø 3,3/3,75/4,2/5/6 Platform: Universal (Code 0040)	p. 26

✱ Internal Hex Connection (IH) NEO	
Implant: Ø 3,75/4,2/5 Platform: 3,5 (Code 0040)	p. 26

✱ Conical Standard Connection (CS)	
Implant: Ø 3,75/4,2/5 Platform: Standard (Code 0169)	p. 30

ANCLADEN

✱ Anclalock	
Implant: Ø 3,75/4,25/5 Platform: 3,5 (Code 0040)	p. 26

ARDS

✱ Smart	
Implant: Ø 3,75/4,2/4,5 Platform: 3,75 (Code 0040)	p. 26

✱ Classic	
Implant: Ø 3,75/4,2/4,5 Platform: 3,75 (Code 0040)	p. 26
Implant: Ø 3,3/3,75/4,2/5/6 Platform: 3,75 (Code 0040)	p. 26

✱ Premium	
Implant: Ø 3,3/3,75/4,2/5/6 Platform: 3,75 (Code 0040)	p. 26

✱ CIT	
Implant: Ø 3,3/3,75/4,2/5/6 Platform: 3,75 (Code 0040)	p. 26

ANKYLOS

✱ Ankylos	
Implant: Ø 3,5 Platform: 3,5 (Code 0075)	p. 27
Implant: Ø 4,5 Platform: 4,5 (Code 0075)	p. 27
Implant: Ø 5,5 Platform: 5,5 (Code 0075)	p. 27
Implant: Ø 7 Platform: 7 (Code 0075)	p. 27

ASTRA

✱ Aqua	
Implant: Ø 3,5/4 Platform: Aqua (Code 0004)	p. 22

✱ Evolution (Internal)	
Implant: Ø 3,6 Platform: 3,6 (Code 0006)	p. 23
Implant: Ø 4,2 Platform: 4,2 (Code 00007)	p. 23
Implant: Ø 4,8 Platform: 4,8 (Code 00091)	p. 27

AVINENT

✱ HI/IC	
Implant: Ø 3,1//3,5/4 Platform: 3,5 (Code 0040)	p. 26

BIOCONCEPT

✱ BC Bone Level	
Implant: Ø 3,3 Platform: Narrow (Code 0033)	p. 25
Implant: Ø 4,1/4,8 Platform: Regular (Code 0035)	p. 26

✱ BV Tapered Bone Level	
Implant: Ø 3,5 Platform: Narrow (Code 0029)	p. 25
Implant: Ø 4/4,5/5 Platform: Regular (Code 0030)	p. 25

BIOHORIZONS

✱ Tapered Internal	
Implant: Ø 3,8 Platform: 3,5 (Yellow) (Code 0040)	p. 26
Implant: Ø 3/3,4 Platform: 3,5 (Grey) (Code 0102)	p. 27

✱ Internal	
Implant: Ø 3,5/4 Platform: 3,5 (Yellow) (Code 0040)	p. 26

BIOMET 3i

✱ Certain	
Implant: Ø 3,25/4 Platform: 3,4 (Code 0001)	p. 22
Implant: Ø 4/5 Platform: 4,1 (Code 0001)	p. 22

BIONER

✱ Hikelt	
Implant: Ø 3,8 Platform: 3,95 (Code 0040)	p. 26

✱ TopDM	
Implant: Ø 3,5 Platform: 3,5 (Code 0021)	p. 24
Implant: Ø 4 Platform: 4 (Code 0021)	p. 24
Implant: Ø 5 Platform: 5 (Code 0021)	p. 24

BIOTEC

✱ SPR/CIM	
Implant: Ø 3,3 Platform: 3,3 (Code 0040)	p. 26
Implant: Ø 3,75 Platform: 3,75 (Code 0040)	p. 26
✱ SPR/SPTT/CIM	
Implant: Ø 4,2 Platform: 4,2 (Code 0040)	p. 26
Implant: Ø 5 Platform: 5 (Code 0040)	p. 26

BTK

✱ Klassic / Konic	
Implant: Ø 3,25/4 Platform: 3,5 IR (Code 0040)	p. 26

B&W

✱ Internal Hexagon CIH	
Implant: Ø 3,3/4 Platform: 4 (Code 0040)	p. 26

CAMLOG

✱ Conelog Screw-Line/Progressive-Line	
Implant: Ø 3,3 Platform: 3,3 (Code 0119)	p. 28
Implant: Ø 3,8 Platform: 3,8 (Code 0120)	p. 28
Implant: Ø 4,3 Platform: 4,3 (Code 0121)	p. 28

CONEXÃO SISTEMA DE PRÓTESE

✱ Flash	
Implant: Ø 3,5/4,3/5 Platform: Universal (Code 0021)	p. 24
✱ Torq	
Implant: Ø 3,5/3,75/4 Platform: Universal (Code 0021)	p. 24
✱ Expand	
Implant: Ø 3,75/4/5 Platform: Universal (Code 0021)	p. 24

CORTEX

✱ Dynamix	
Implant: Ø 3,3/3,8/4,2/5/6 Platform: 3,75 (Code 0040)	p. 26
✱ Classix	
Implant: Ø 3,3/3,8/4,2/5/6 Platform: 3,75 (Code 0040)	p. 26
✱ Saturn	
Implant: Ø 3,8/4,2 Platform: 3,5 (Code 0040)	p. 26

✱ Conical Platform:	
Implant: Ø 3,3/3,8/4,2 Platform: RP (Code 0004)	p. 22

✱ Magix	
Implant: Ø 3,3/3,8/4,2 Platform: RP (Code 0004)	p. 22

DENTIS

✳️ s-Clean	
Implant: Ø 3,7 Platform: Mini (Code 0030)	p. 25
Implant: Ø 4,1/4,3 Platform: Regular (Code 0030)	p. 25
Implant: Ø 4,8 Platform: Wide (Code 0030)	p. 25

DENTIUM

✳️ SuperLine and Implantium	
Implant: Ø 3,4 Platform: 3,6 (Code 0030)	p. 25
Implant: Ø 3,8 Platform: 4 (Code 0030)	p. 25
Implant: Ø 4,3 Platform: 4,5 (Code 0030)	p. 25
Implant: Ø 4,8 Platform: 5 (Code 0030)	p. 25
Implant: Ø 4,8 Platform: 6 (Code 0030)	p. 25

DIO IMPLANTS

✳️ UF II	
Implant: Ø 3,8/4/4,5/5/5,5 Platform: Regular (Code 0030)	p. 25
✳️ UF II Narrow	
Implant: Ø 3 / 3,3 Platform: Narrow (Code 0014)	p. 23

EASY IMPLANT

✳️ Master C	
Implant: Ø 3,5 Platform: 3,5 (Ocean) (Code 0004)	p. 22
Implant: Ø 4 Platform: 4 (Ocean) (Code 0004)	p. 22

Implant: Ø 4,5 Platform: 4,5 (Lilas) (Code 0030)	p. 25
Implant: Ø 5 Platform: 5 (Lilas) (Code 0030)	p. 25

✳️ Master S	
Implant: Ø 3,3 Platform: 3,3 (Ocean) (Code 0004)	p. 22
Implant: Ø 3,75 Platform: 3,75 (Lilas) (Code 0030)	p. 25
Implant: Ø 4,25 Platform: 4,25 (Lilas) (Code 0030)	p. 25
Implant: Ø 4,75 Platform: 4,75 (Lilas) (Code 0030)	p. 25

✳️ Master L	
Implant: Ø 3,3 Platform: 3,3 (Lilas) (Code 0030)	p. 25
Implant: Ø 3,75 Platform: 3,75 (Lilas) (Code 0030)	p. 25
Implant: Ø 4,25 Platform: 4,25 (Lilas) (Code 0030)	p. 25
Implant: Ø 4,75 Platform: 4,75 (Lilas) (Code 0030)	p. 25

EUROTEKNIKA

✳️ Naturactis	
Implant: Ø 3,5 Platform: 3,4 (Code 0004)	p. 22
Implant: Ø 4 Platform: 3,8 (Code 0004)	p. 22
Implant: Ø 4,5 Platform: 4,3 (Code 0004)	p. 22
Implant: Ø 5 Platform: 4,8 (Code 0004)	p. 22

✳️ Natea	
Implant: Ø 3,6/4,1/4,8 Platform: Narrow (Code 0004)	p. 22
Implant: Ø 3,6/4,1/4,8 Platform: Regular (Code 0004)	p. 22
Implant: Ø 6 Platform: Wide (Code 0004)	p. 22

✳️ Naturall	
Implant: Ø 3,5 Platform: Narrow (Code 0004)	p. 22
Implant: Ø 4/4,5 Platform: Regular (Code 0004)	p. 22
Implant: Ø 5 Platform: Wide (Code 0004)	p. 22

GALIMPLANT

✳️ Internal Connection	
Implant: Ø 3,5 Platform: 3,5 (Code 0004)	p. 22
Implant: Ø 4 Platform: 4 (Code 0004)	p. 22
Implant: Ø 5 Platform: 5 (Code 0004)	p. 22

GLOBAL D (TEKKA)

✳️ In-Kone Universal	
Implant: Ø 3,5/4/4,5/5 Platform: Universal (Code 0152)	p. 29

HAHN IMPLANT (GLIDEWELL)

✳️ Hahn Tapered Implant	
Implant: Ø 3,5/4,3 Platform: 3,5/4,3 (Code 0021)	p. 24
Implant: Ø 5 Platform: 5 (Code 0022)	p. 24

HI-TEC

✳️ Tapered Self Thread	
Implant: Ø 3,3/3,75 Platform: 3,5 (Code 0040)	p. 26
✳️ Logic Plus	
Implant: Ø 3,5 Platform: 3,7 (Code 0040)	p. 26
Implant: Ø 4,3 Platform: 3,9 (Code 0040)	p. 26

HIOSSEN

✳️ ETTI SA/ETIII SA	
Implant: Ø 3,5 Platform: Mini (Code 0029)	p. 25
Implant: Ø 4/4,5/5 Platform: Regular (Code 0030)	p. 25
✳️ ETTI BA	
Implant: Ø 3,5 Platform: Mini (Code 0029)	p. 25
Implant: Ø 4/4,5/5 Platform: Regular (Code 0030)	p. 25

IBS

✳️ Magic FC	
Implant: Ø 4/4,5/5/5,5/6/6,5 Platform: 3,8 (Code 0030)	p. 25
✳️ N.R Fix	
Implant: Ø 3/3,5 Platform: 3,8 (Code 0030)	p. 25

IDO IMPLANTS

✳️ IDo Implant	
Implant: Ø 3,8/4/4,5/5/5,5/6/7 Platform: Universal (Code 0030)	p. 25

IHDE DENTAL (IMBIODENT)

✳️ Bone Level Plus	
Implant: Ø 3,3 Platform: 3,3 (Code 0033)	p. 25
Implant: Ø 4,1 Platform: 4,1 (Code 0035)	p. 26
Implant: Ø 4,8 Platform: 4,8 (Code 0035)	p. 26

IMPLANT DIRECT

✳️ Legacy	
Implant: Ø 3,7/4,2 Platform: 3,5 (Code 0040)	p.26
✳️ SwishActive	
Implant: Ø 3,3 Platform: 3 (Code 0021)	p. 24
Implant: Ø 4,1/4,8 Platform: 3,4 (Code 0022)	p. 24
✳️ Interactive	
Implant: Ø 3,2/3,7 Platform: 3 (Code 0021)	p. 24
Implant: Ø 4,3/5 Platform: 3,4 (Code 0022)	p. 24

IMPLANT GENESIS

✳️ Aktiv System	
Implant: Ø 3,5/3,75/4,2/5 Platform: Standard (Code 0040)	p. 26

INTRA-LOCK

✳️ IntraHex	
Implant: Ø 3,75/4 Platform: 3,5 (Code 0040)	p. 26

JDENTALCARE

✳️ JDEvolution/JDEvolution Plus	
Implant: Ø 3,7 Platform: 3,7 (Code 0040)	p. 26
Implant: Ø 4,3/5 Platform: 4 (Code 0040)	p. 26
Implant: Ø 6 Platform: 5 (Code 0040)	p. 26
✳️ JD ICON	
Implant: Ø 3,9 Platform: 3,9 (Code 0022)	p. 24
Implant: Ø 4,3 Platform: 4 (Code 0022)	p. 24
Implant: Ø 5 Platform: 4,7 (Code 0022)	p. 24

LEADER

✳️ Tixos Internal Hex	
Implant: Ø 3,3 Platform: 3,5 (Code 0040)	p. 26
Implant: Ø 3,75 Platform: 4 (Code 0040)	p. 26

MEDENTIS

✳️ ICX - Templant	
Implant: Ø 3,75 Platform: 3,75 (Code 0125)	p. 29
Implant: Ø4,1 Platform: 4,1 (Code 0125)	p. 29
Implant: Ø 4,8 Platform: 4,8 (Code 0125)	p. 29

MEGAGEN

- AnyRidge
  - Implant: Ø 3,5
  - Platform: Small (Code 0015) p. 24
- Implant: Ø 4/4,5
  - Platform: Regular (Code 0015) p. 24
- Implant: Ø 5/5,5
  - Platform: Wide (Code 0015) p. 24
- AnyOne Internal
  - Implant: Ø 3,5/4/4,5/5/6/7
  - Platform: General (Code 0030) p. 25
- Mini Narrow Ridge
  - Implant: Ø 3 / 3,4
  - Platform: Mini (Code 0014) p. 23

MIS

- Seven
  - Implant: Ø 3,75/4,2
  - Platform: Standard (Code 0040) p. 26
- M4
  - Implant: Ø 3,75/4,2
  - Platform: Standard (Code 0040) p. 26

MOZO-GRAU

- MG Inhex
  - Implant: Ø 3,75/4,25
  - Platform: 2,8 Standard (Code 0004) p. 22

MPI

- Privilege CM
  - Implant: Ø 3,5/4
  - Platform: Regular (Code 0004) p. 22
- Excellence CM
  - Implant: Ø 3,5/4
  - Platform: Regular (Code 0004) p. 22

NEODENT

- Helix GM/Drive GM/ Titamax GM
  - Implant: Ø 3,5/3,75/4/4,3/5/6
  - Platform: Regular (Code 0186) p. 29

NEOBIOTECH

- IS Implant: System
  - Implant: Ø 4
  - Platform: Regular 4 (Code 0030) p. 25
- Implant: Ø 4,5
  - Platform: Regular 4,5 (Code 0030) p. 25
- Implant: Ø 5
  - Platform: Wide 5 (Code 0030) p. 25

NOBEL BIOCARE

- Active
  - Implant: Ø 3,5
  - Platform: Narrow (Code 0021) p. 24
- Implant: Ø 4,3/5
  - Platform: Regular (Code 0022) p. 24
- NobelParallel
  - Implant: Ø 3,75
  - Platform: Narrow (Code 0021) p. 24
- Implant: Ø 4,3/5
  - Platform: Regular (Code 0022) p. 24

NORIS MEDICAL

- Tuff
  - Implant: Ø 3,3/3,75/4,2/5/6
  - Platform: 3,75 (Code 0040) p. 26
- Tuff TT
  - Implant: Ø 3,3/3,75/4,2/5/6
  - Platform: 3,75 (Code 0040) p. 26
- Onix
  - Implant: Ø 3,3/3,75/4,2/5/6
  - Platform: 3,75 (Code 0040) p. 26

- Cortical
  - Implant: Ø 4,0/5/6
  - Platform: 3,75 (Code 0040) p. 26

- PteryCore
  - Implant: Ø 4,2
  - Platform: 3,75 (Code 0040) p. 26

- PteryFit
  - Implant: Ø 4,2
  - Platform: 3,75 (Code 0040) p. 26

OSTEOPLUS

- Shi
  - Implant: Ø 3,3 / 3,75 / 4,2
  - Platform: 3,5 (Code 0040) p. 26

OSSTEM IMPLANT

- TS
  - Implant: Ø 3,5
  - Platform: Mini (Code 0029) p. 25
- Implant: Ø 4/4,5/5/6/7
  - Platform: Regular (Code 0030) p. 25

PALTOP

- Conical Active
  - Implant: Ø 3,75/4,2/5
  - Platform: Standard (Code 0029) p. 25

PROCLINIC

- Aqua CM
  - Implant: Ø 3,5/4/5
  - Platform: 2,82 (Code 0004) p. 22
- Cylindrical Internal/Conical Internal
  - Implant: Ø 3,3/3,75/4,25/5//3,5/4/5
  - Platform: 3,5 (Code 0040) p. 26

SEWON MEDIX

- IH2 SLA SYSTEM
  - Implant: Ø 3,5
  - Platform: Mini (Code 0029) p. 25
- Implant: Ø 3,5/4/4,5/5
  - Platform: Regular (Code 0030) p. 25

IH2 RBM SYSTEM

- Implant: Ø 3,5
  - Platform: Mini (Code 0029) p. 25
- Implant: Ø 3,5/4/4,5/5
  - Platform: Regular (Code 0030) p. 25

SGS

- P1
  - Implant: Ø 3,2/3,75/4,2/5/6
  - Platform: 3,75 (Code 0040) p. 26
- P7
  - Implant: Ø 3,2/3,75/4,2/4,5/5/6
  - Platform: 3,75 (Code 0040) p. 26

SIGNO VINCES

- Compact
  - Implant: Ø 4,5
  - Platform: CM3,8 (Code 0004) p. 22
- Duocon
  - Implant: Ø 3,8
  - Platform: CM3,8 (Code 0004) p. 22
- Infra
  - Implant: Ø 3,3/3,8/4,6
  - Platform: CM (Code 0004) p. 22

SIN IMPLANTS

- HI SW
  - Implant: Ø 3,8
  - Platform: 3,8 (Code 0039) p. 26

SOUTHERN IMPLANTS

- Deep Conical
  - Implant: Ø 3,5/4
  - Platform: 2,95/3,1 (Code 0004) p. 22
- Internal Hex
  - Implant: Ø 3,75/4,2/5
  - Platform: Universal (Code 0040) p. 26

STRAUMANN

- Bone Level
  - Implant: Ø 3,3
  - Platform: NC- 3,3 (Code 0033) p. 25
- Implant: Ø 4,1
  - Platform: RC-4,1 (Code 0035) p. 26
- Implant: Ø 4,8
  - Platform: RC-4,8 (Code 0035) p. 26
- BLX
  - Implant: Ø 3,5/3,75/4/4,5
  - Platform: RB (Regular Base) (Code 0207) p. 30

TITANIUM-FIX

- b-fix
  - Implant: Ø 3,5/4
  - Platform: Regular (Code 0004) p. 22

TRE-OSS

- Simple
  - Implant: Ø 3,3/3,75/5
  - Platform: 3,75 Amarillo (Code 0040) p. 26

TRI DENTAL IMPLANTS

- TRI-Vent
  - Implant: Ø 3,75/4,1/4,7
  - Platform: 3,5 (Code 0040) p. 26

UFIT

- Gt2
  - Implant: Ø 3,5
  - Platform: Mini (Code 0004) p. 22
- Nt2
  - Implant: Ø 3,5
  - Platform: Mini (Code 0004) p. 22

VULKAN IMPLANTS

- IN-Hex
  - Implant: Ø 3,3/3,75/4,2/5
  - Platform: 3,75 (Code 0040) p. 26

XIVE

- Xive
  - Implant: Ø 3,8
  - Platform: 3,8 (Code 0039) p. 26

YES IMPLANT

- S-SYSTEM
  - Implant: Ø 3,3/3,5
  - Platform: Narrow (Code 0030) p. 25
- Implant: Ø 4/4,5
  - Platform: Regular (Code 0030) p. 25
- Implant: Ø 5/5,5
  - Platform: Wide (Code 0030) p. 25


ZIMMER

- Screw-Vent
  - Implant: Ø 3,7/4,1
  - Platform: 3,5 (Code 0040) p. 26

COMPATIBLE with 0001

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.302.001.01-2	42.302.001.02-2	42.302.001.03-2	42.302.001.04-2


**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_4.5\_0001\_PREMIUM  
DAS\_MU\_8\_0001\_PREMIUM  
DAS\_MU\_DS8\_0001\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0001\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0001\_PREMIUM

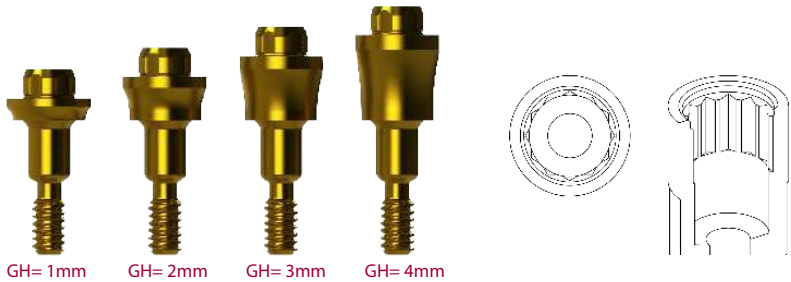

COMPATIBLE with 0002

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.303.002.01-2	42.303.002.02-2	42.303.002.03-2	42.303.002.04-2


**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_4.5\_0002\_PREMIUM  
DAS\_MU\_8\_0002\_PREMIUM  
DAS\_MU\_DS8\_0002\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0002\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0002\_PREMIUM

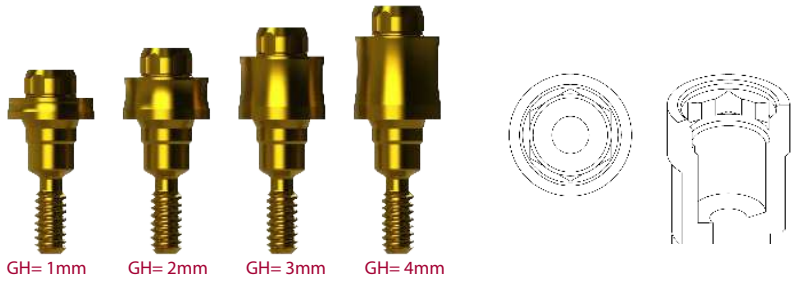

COMPATIBLE with 0004

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.303.004.01-2	42.303.004.02-2	42.303.004.03-2	42.303.004.04-2


**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_4.5\_0004\_PREMIUM  
DAS\_MU\_8\_0004\_PREMIUM  
DAS\_MU\_DS8\_0004\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0004\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0004\_PREMIUM

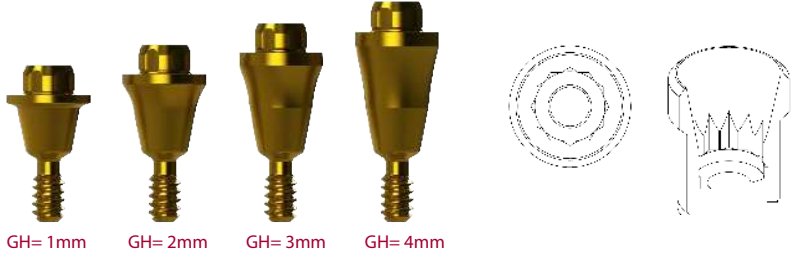

COMPATIBLE with 0006

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.302.006.01-2	42.302.006.02-2	42.302.006.03-2	42.302.006.04-2


**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_4.5\_0006\_PREMIUM  
DAS\_MU\_8\_0006\_PREMIUM  
DAS\_MU\_DS8\_0006\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0006\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0006\_PREMIUM

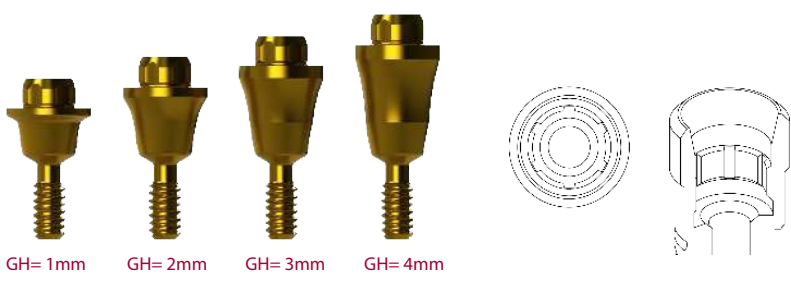

COMPATIBLE with 0007

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.303.007.01-2	42.303.007.02-2	42.303.007.03-2	42.303.007.04-2

**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_4.5\_0007\_PREMIUM  
DAS\_MU\_8\_0007\_PREMIUM  
DAS\_MU\_DS8\_0007\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0007\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0007\_PREMIUM

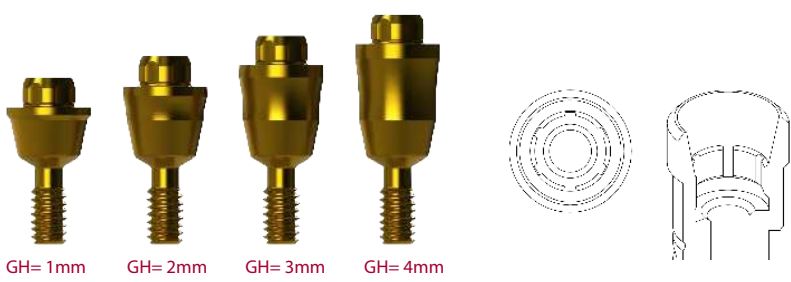

COMPATIBLE with 0014

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	-	42.302.014.02-2	42.302.014.03-2	42.302.014.04-2


**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_4.5\_0014\_PREMIUM  
DAS\_MU\_8\_0014\_PREMIUM  
DAS\_MU\_DS8\_0014\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0014\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0014\_PREMIUM



COMPATIBLE with 0015

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.303.015.01-2	42.303.015.02-2	42.303.015.03-2	42.303.015.04-2


**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_4.5\_0015\_PREMIUM  
DAS\_MU\_8\_0015\_PREMIUM  
DAS\_MU\_DS8\_0015\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0015\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0015\_PREMIUM

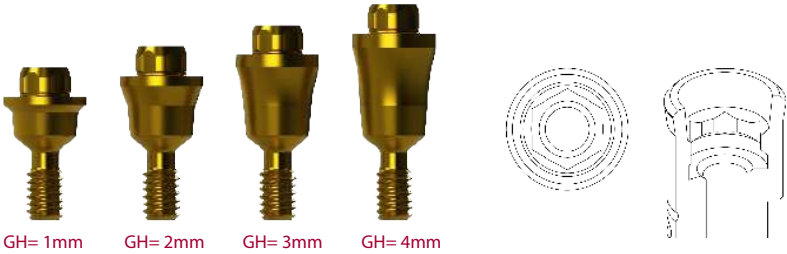

COMPATIBLE with 0021

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.302.021.01-2	42.302.021.02-2	42.302.021.03-2	42.302.021.04-2


**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_4.5\_0021\_PREMIUM  
DAS\_MU\_8\_0021\_PREMIUM  
DAS\_MU\_DS8\_0021\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0021\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0021\_PREMIUM

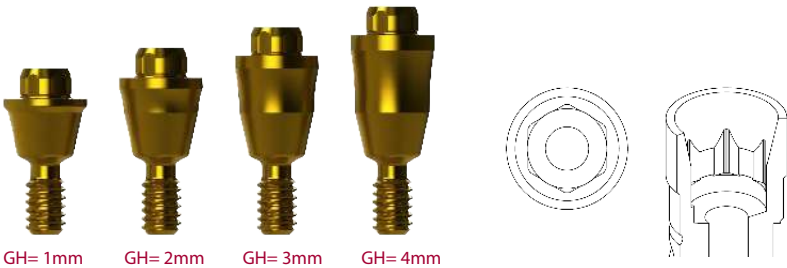

COMPATIBLE with 0022

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.303.022.01-2	42.303.022.02-2	42.303.022.03-2	42.303.022.04-2


**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_4.5\_0022\_PREMIUM  
DAS\_MU\_8\_0022\_PREMIUM  
DAS\_MU\_DS8\_0022\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0022\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0022\_PREMIUM

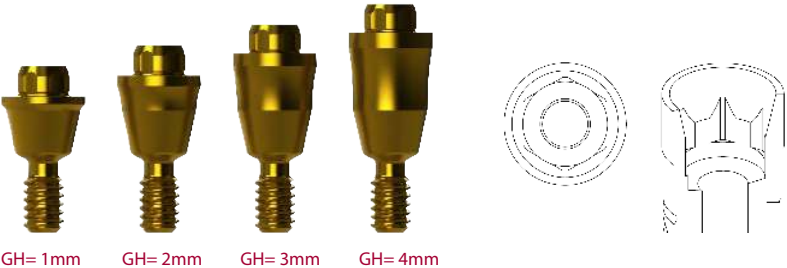

COMPATIBLE with 0029

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.302.029.01-2	42.302.029.02-2	42.302.029.03-2	42.302.029.04-2


**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_4.5\_0029\_PREMIUM  
DAS\_MU\_8\_0029\_PREMIUM  
DAS\_MU\_DS8\_0029\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0029\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0029\_PREMIUM

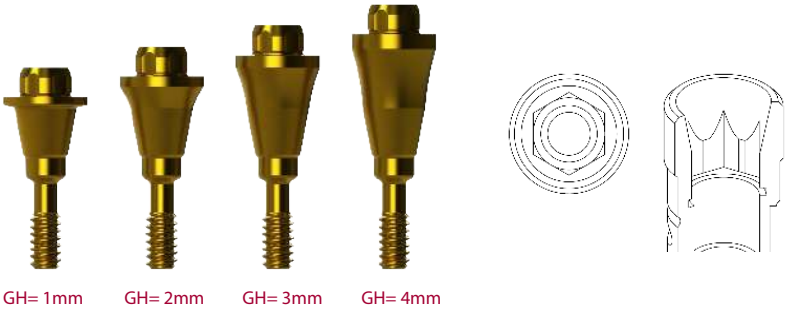

COMPATIBLE with 0030

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.303.030.01-2	42.303.030.02-2	42.303.030.03-2	42.303.030.04-2


**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_4.5\_0030\_PREMIUM  
DAS\_MU\_8\_0030\_PREMIUM  
DAS\_MU\_DS8\_0030\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0030\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0030\_PREMIUM

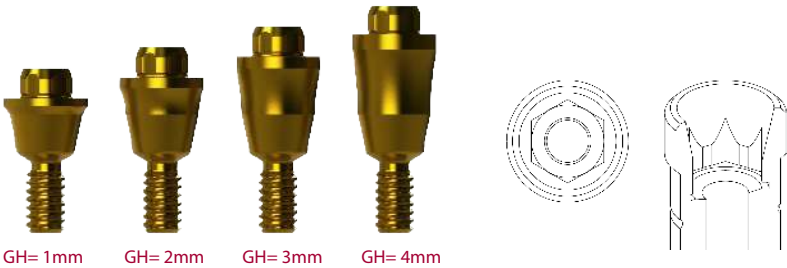

COMPATIBLE with 0033

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.302.033.01-2	42.302.033.02-2	42.302.033.03-2	42.302.033.04-2


**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_4.5\_0033\_PREMIUM  
DAS\_MU\_8\_0033\_PREMIUM  
DAS\_MU\_DS8\_0033\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0033\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0033\_PREMIUM

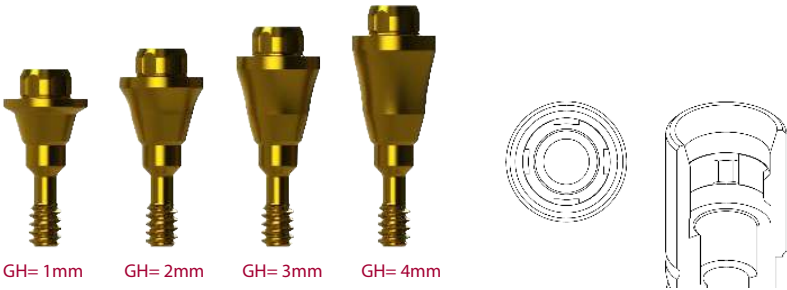

COMPATIBLE with 0035

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.303.035.01-2	42.303.035.02-2	42.303.035.03-2	42.303.035.04-2

**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_4.5\_0035\_PREMIUM  
DAS\_MU\_8\_0035\_PREMIUM  
DAS\_MU\_DS8\_0035\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0035\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0035\_PREMIUM

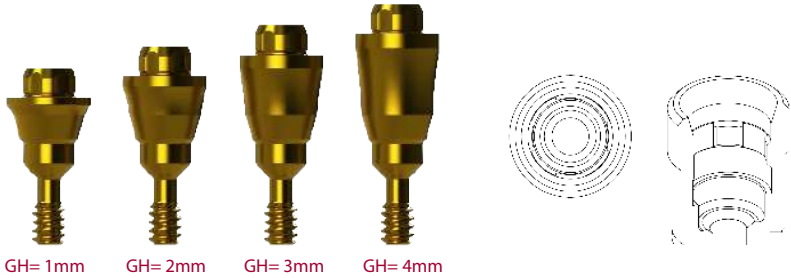

COMPATIBLE with 0039

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.303.039.01-2	-	-	-


**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_4.5\_0039\_PREMIUM  
DAS\_MU\_8\_0039\_PREMIUM  
DAS\_MU\_DS8\_0039\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0039\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0039\_PREMIUM



COMPATIBLE with 0040

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.302.040.01-2	42.302.040.02-2	42.302.040.03-2	42.302.040.04-2

**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_4.5\_0040\_PREMIUM  
DAS\_MU\_8\_0040\_PREMIUM  
DAS\_MU\_DS8\_0040\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0040\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0040\_PREMIUM

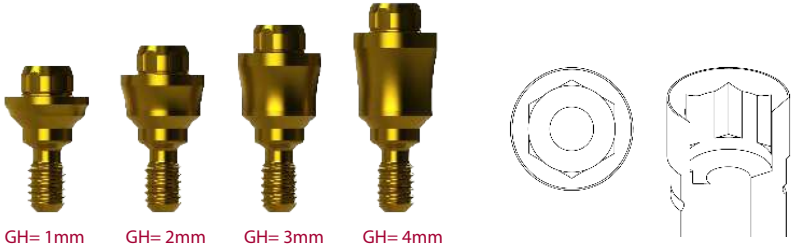

COMPATIBLE with 0075

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	-	42.302.075.02-2	42.302.075.03-2	42.302.075.04-2


**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_4.5\_0075\_PREMIUM  
DAS\_MU\_8\_0075\_PREMIUM  
DAS\_MU\_DS8\_0075\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0075\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0075\_PREMIUM



COMPATIBLE with 0091

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.303.091.01-2	42.303.091.02-2	42.303.091.03-2	42.303.091.04-2


**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_4.5\_0091\_PREMIUM  
DAS\_MU\_8\_0091\_PREMIUM  
DAS\_MU\_DS8\_0091\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0091\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0091\_PREMIUM

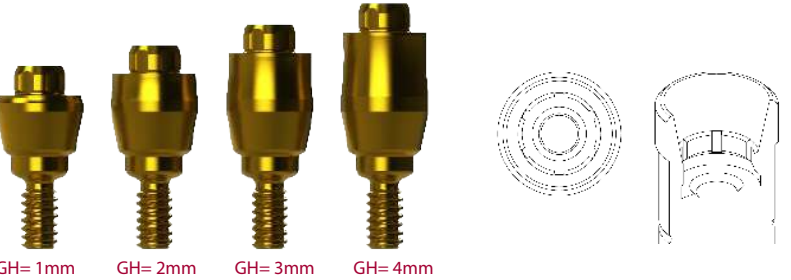

COMPATIBLE with 0102

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.302.102.01-2	42.302.102.02-2	42.302.102.03-2	42.302.102.04-2

**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_4.5\_0102\_PREMIUM  
DAS\_MU\_8\_0102\_PREMIUM  
DAS\_MU\_DS8\_0102\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0102\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0102\_PREMIUM

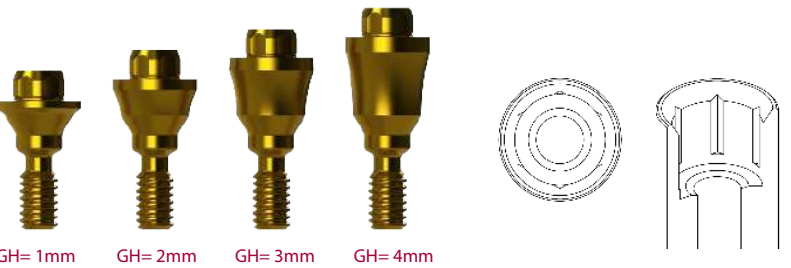

COMPATIBLE with 0119

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.301.119.01-2	42.301.119.02-2	42.301.119.03-2	42.301.119.04-2

DAS LIBRARIES:

MU SCANBODY DAS\_MU\_4.5\_0119\_PREMIUM  
DAS\_MU\_8\_0119\_PREMIUM  
DAS\_MU\_DS8\_0119\_PREMIUM

MU SCANALOG DAS\_MU\_SA\_0119\_PREMIUM

DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0119\_PREMIUM



GH= 1mm GH= 2mm GH= 3mm GH= 4mm

COMPATIBLE with 0120

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.303.121.01-2	42.303.121.02-2	42.303.121.03-2	42.303.121.04-2

DAS LIBRARIES:

MU SCANBODY DAS\_MU\_4.5\_0120\_PREMIUM  
DAS\_MU\_8\_0120\_PREMIUM  
DAS\_MU\_DS8\_0120\_PREMIUM

MU SCANALOG DAS\_MU\_SA\_0120\_PREMIUM

DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0120\_PREMIUM



GH= 1mm GH= 2mm GH= 3mm GH= 4mm

COMPATIBLE with 0121

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.303.121.01-2	42.303.121.02-2	42.303.121.03-2	42.303.121.04-2

DAS LIBRARIES:

MU SCANBODY DAS\_MU\_4.5\_0121\_PREMIUM  
DAS\_MU\_8\_0121\_PREMIUM  
DAS\_MU\_DS8\_0121\_PREMIUM

MU SCANALOG DAS\_MU\_SA\_0121\_PREMIUM

DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0121\_PREMIUM



GH= 1mm GH= 2mm GH= 3mm GH= 4mm

COMPATIBLE with 0125


MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.303.125.01-2	42.303.125.02-2	42.303.125.03-2	42.303.125.04-2

DAS LIBRARIES:

MU SCANBODY DAS\_MU\_4.5\_0125\_PREMIUM  
DAS\_MU\_8\_0125\_PREMIUM  
DAS\_MU\_DS8\_0125\_PREMIUM

MU SCANALOG DAS\_MU\_SA\_0125\_PREMIUM

DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0125\_PREMIUM

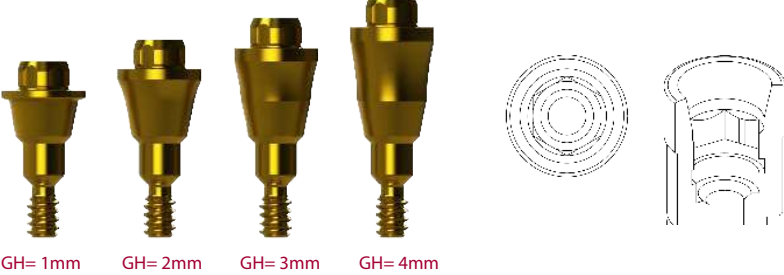

GH= 1mm GH= 2mm GH= 3mm GH= 4mm

COMPATIBLE with 00152


MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	-	42.300.152.03-2	42.300.152.02-2	-

DAS LIBRARIES:

MU SCANBODY DAS\_MU\_4.5\_0152\_PREMIUM  
DAS\_MU\_8\_0152\_PREMIUM  
DAS\_MU\_DS8\_0152\_PREMIUM

MU SCANALOG DAS\_MU\_SA\_0152\_PREMIUM

DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0152\_PREMIUM

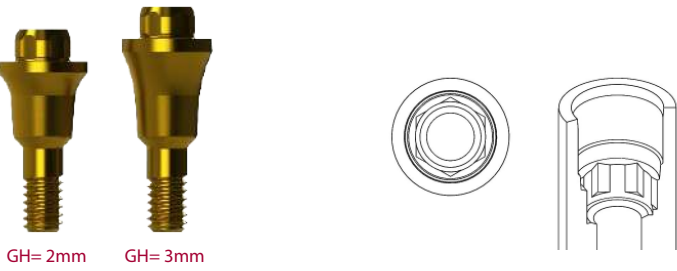

GH= 2mm GH= 3mm

COMPATIBLE with 0186

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.303.186.01-2	42.303.186.02-2	42.303.186.03-2	42.303.186.04-2

DAS LIBRARIES:

MU SCANBODY DAS\_MU\_4.5\_0186\_PREMIUM  
DAS\_MU\_8\_0186\_PREMIUM  
DAS\_MU\_DS8\_0186\_PREMIUM

MU SCANALOG DAS\_MU\_SA\_0186\_PREMIUM

DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0186\_PREMIUM



GH= 1mm GH= 2mm GH= 3mm GH= 4mm

COMPATIBLE with 0169

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.302.169.01-2	42.302.169.02-2	42.302.169.03-2	42.302.169.04-2

**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_0169\_PREMIUM  
DAS\_MU\_8\_0169\_PREMIUM  
DAS\_MU\_DS8\_0169\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0169\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0169\_PREMIUM



COMPATIBLE with 0207

MULTI-UNIT				
	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT	GINGIVAL HEIGHT
	1 mm	2 mm	3 mm	4 mm
R	42.302.207.01-2	42.302.207.02-2	42.302.207.03-2	42.302.207.04-2

**DAS LIBRARIES:**  
MU SCANBODY DAS\_MU\_0207\_PREMIUM  
DAS\_MU\_8\_0207\_PREMIUM  
DAS\_MU\_DS8\_0207\_PREMIUM  
MU SCANALOG DAS\_MU\_SA\_0207\_PREMIUM  
DYNAMIC μSCANBODY DAS\_MU\_I/IG\_0207\_PREMIUM



TALLADIUM GUARANTEE

**TERMS AND CONDITIONS**  
These guarantee terms and conditions (“T&C”) cover the entire range of Talladium products (“Products”), manufactured by TALLADIUM ESPAÑA S.L. and distributed by Geoda Medical S.L. or official dealers. The guarantee described in these T&C is exclusively in benefit of the clinician (“Clinician”) and of the dental technician (“Technician”) and not for the benefit of third parties or institutions, including patients.

**GUARANTEE PERIOD**  
TALLADIUM ESPAÑA S.L. offers a lifelong guarantee for its entire range of products starting from the date of issue of the invoice.

**GUARANTEE SCOPE**  
Subject to the limitations and exceptions described in these T&C, TALLADIUM ESPAÑA S.L. will offer the following benefits:

**QUALITY:** If there are defects in the materials or in the manufacturing of the Product, TALLADIUM ESPAÑA S.L. will replace the Product with no additional cost.

**SAFETY:** If, having complied with all the product indications, the prosthesis should have to be made again, due to a fault in the Dynamic Abutment® or Dynamic Titanium Base® system, TALLADIUM ESPAÑA S.L. will replace the abutments and screws necessary to remake the prosthesis, as well as the costs derived from its manufacturing.

In case of having used our products and having complied with all the product indications, the implants suffer any damage, TALLADIUM ESPAÑA S.L. will pay the cost of the implants. This coverage will only be valid during the first 6 months after the collocation of the prosthesis which includes our products.

- CLAIM REQUIREMENTS AND PROCEDURE**  
To receive the benefits indicated in these T&C, the treating Clinician must satisfy the following requirements:
- a) The claim must be notified to TALLADIUM ESPAÑA S.L. within (30) days since the date the claimed defect was detected.
  - b) This requires that the Clinician or Technician must contact the customer service department by telephone or by e-mail to make the claim.
  - c) A claim form will be completed, which, together with a document or report which justifies the faulty Product and the faulty Product itself, will be sent by the customer to TALLADIUM ESPAÑA S.L. offices, within the previously indicated period.
  - d) Clinicians or Technicians presenting a claim in agreement with these T&C must be up to date in any payments owing to TALLADIUM ESPAÑA S.L. or to any of its subsidiaries, at the time when the claim form is presented.
  - e) All the use procedures of our Products must be carried out in agreement with the instructions of TALLADIUM ESPAÑA S.L. as well as in accordance with commonly accepted dentistry practices.
  - f) The expenses derived from this procedure will be assumed by the customer. The return shipping costs will be assumed by TALLADIUM ESPAÑA S.L. in all those cases covered by these T&C.

Regardless of the guarantee rights, claims should be notified as soon as possible in order to comply with regulatory requirements.

**GENERAL LIMITATIONS OF THIS GUARANTEE**  
With the exception of the guarantee described in these T&C, neither TALLADIUM ESPAÑA S.L. nor its representatives, nor third parties manufacturing or distributing the Products, represent or offer a guarantee, agreement or any other express or implicit, oral or written, commitment, with respect to the Products (without limitation), including guarantees involved in the marketing, durability or suitability for individual uses or purposes.

In addition and within the maximum extent permitted by the relative law, TALLADIUM ESPAÑA S.L. rejects (on its own behalf, and on behalf of its representatives and third parties that manufacture or distribute Products) any responsibility with respect to any direct or indirect damage caused, which may result from or be a consequence of the design, composition of the dental prosthesis into which the Products are integrated.

**GUARANTEE EXCLUSIONS**  
TALLADIUM ESPAÑA S.L. limits this guarantee to:

- Transformed abutments that form part of the dental prosthesis. But not the screws used to anchor them.
- Clinical screws that have been in the mouth for more than 2 years.

**AMENDMENT OR SUSPENSION OF THE GUARANTEE**  
TALLADIUM ESPAÑA S.L. reserves the right to amend or withdraw these T&C at any time and without prior notification. Any modification or suspension shall not affect products already placed in patients.